


Column : AppliChrom SugarSep-H V; 300mm x8mm; P/N SASHV103008 Detection : RI
 Mobile Phase : H2O/0.1% H2SO4 Temperature : 60C
 Flow Rate : 0.6 mL/min Pressure : -
 Note : Sample Test Mix M49 / Organic Acids

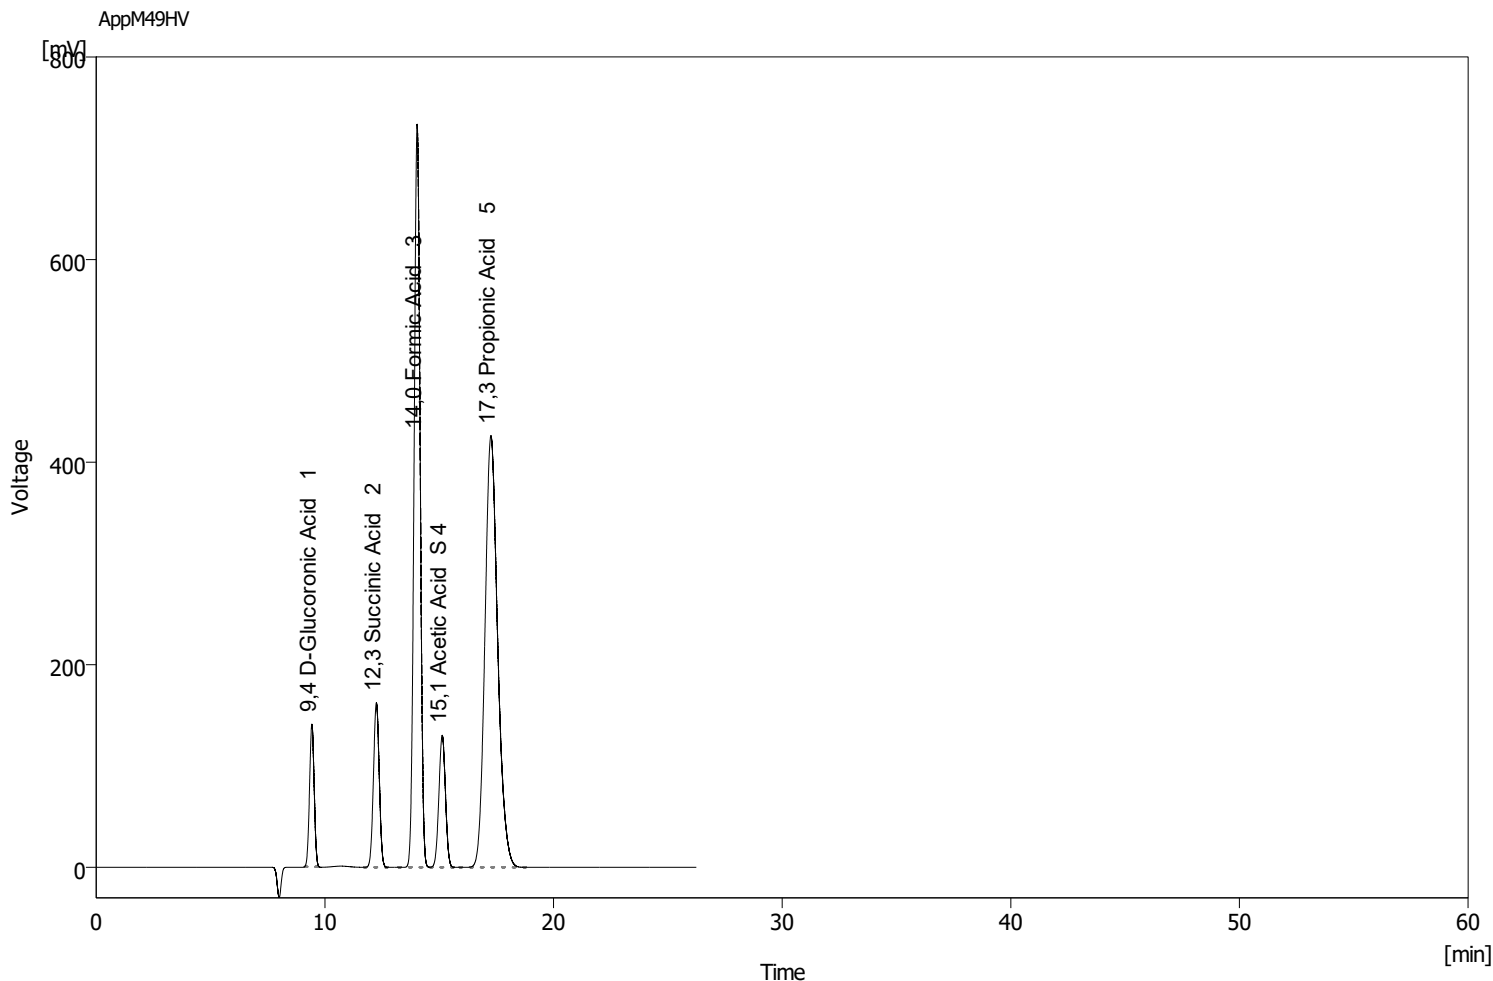

Clarity Lite - 15.08.2023 14_22_43

	Reten. Time [min]	Compound Name	Asymmetry [-]	Efficiency [th.pl]	Eff/I [t.p./m]	Resolution [-]
1	9,430	D-Glucoronic Acid	1,002	9877	32923	
2	12,251	Succinic Acid	1,003	10733	35776	6,635
3	14,035	Formic Acid	1,001	12976	43253	3,704
4	15,130	Acetic Acid	1,001	12849	42830	2,139
5	17,261	Propionic Acid	1,290	4768	15894	2,785